

# External Trigger TTL input

## Quick Guide

### 1. Intended use


The External Trigger TTL input has been designed to allow the connection of a TTL wired signal to represent a signal into an EEG channel for the Enobio or StarStim devices.

### 2. Safety Information

The TTL external trigger input, ensures the isolation of the subject following the norms:

- UNE-EN 60601-1:1993 + A1:1996 + A2:1996 + A3:1997 + A2/ERR:1999
- UNE-EN 60601-1-2:2008
- UNE-EN 60601-2-26:2004

### 3. Connections to the device

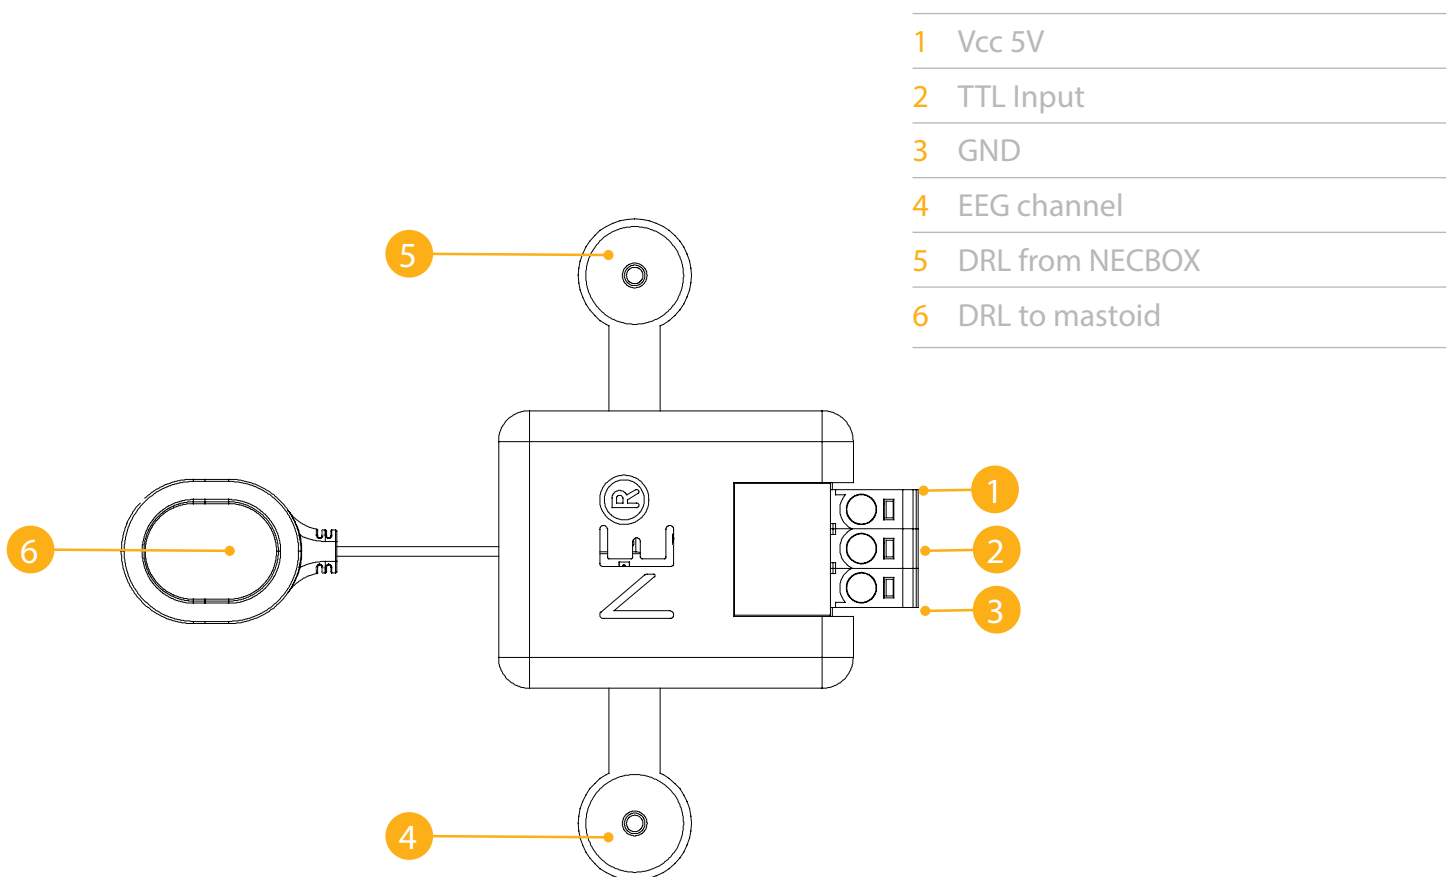

NE  
neuroelectrics®

Avinguda Tibidabo, 47 bis  
08030 Barcelona, Spain  
Tel.+34 93 254 03 63

210 Broadway, Suite 201  
Cambridge, MA 02139, USA  
Tel: +1 617 682 0770

[info@www.neuroelectrics.com](mailto:info@www.neuroelectrics.com)  
[www.neuroelectrics.com](http://www.neuroelectrics.com)

